

See discussions, stats, and author profiles for this publication at: <https://www.researchgate.net/publication/314174662>

Five-year follow-up of underexpanded and overexpanded bioresorbable scaffolds: self-correction and...

Article in *EuroIntervention: journal of EuroPCR in collaboration with the Working Group on Interventional Cardiology of the European Society of Cardiology* · March 2017

DOI: 10.4244/EIJ-D-17-00081

CITATIONS

0

READS

83

11 authors, including:



Yohei Sotomi

Osaka Police Hospital

141 PUBLICATIONS 413 CITATIONS

[SEE PROFILE](#)



Yoshinobu Onuma

Erasmus MC

539 PUBLICATIONS 11,037 CITATIONS

[SEE PROFILE](#)



Andrew Ooi

University of Melbourne

221 PUBLICATIONS 1,877 CITATIONS

[SEE PROFILE](#)



Patrick W Serruys

Erasmus MC / Imperial College London

3,700 PUBLICATIONS 136,505 CITATIONS

[SEE PROFILE](#)

Some of the authors of this publication are also working on these related projects:



Determining the academic approach to developing communication skills in engineering students.

[View project](#)



Study of turbulence-driven secondary flow [View project](#)

Five-year follow-up of underexpanded and overexpanded bioresorbable scaffolds: self-correction and impact on shear stress



Ryo Torii¹, PhD; Erhan Tenekecioglu², MD; Christos Bourantas^{3,4}, MD, PhD; Eric Poon⁵, PhD; Vikas Thondapu^{5,6}, MD; Frank Gijzen⁷, PhD; Yohei Sotomi⁸, MD; Yoshinobu Onuma², MD, PhD; Peter Barlis⁶, MD, PhD; Andrew S.H. Ooi⁵, PhD; Patrick W. Serruys^{2,9*}, MD, PhD

1. Department of Mechanical Engineering, University College London, London, United Kingdom; 2. Department of Interventional Cardiology, Erasmus University Medical Center, Thoraxcenter, Rotterdam, The Netherlands; 3. Department of Cardiology, Barts Heart Centre, London, United Kingdom; 4. Institute of Cardiovascular Sciences, University College London, London, United Kingdom; 5. Department of Mechanical Engineering, Melbourne School of Engineering, University of Melbourne, Melbourne, Australia; 6. Melbourne Medical School, Faculty of Medicine, Dentistry & Health Sciences, University of Melbourne, Melbourne, Australia; 7. Department of Biomedical Engineering, Erasmus University Medical Center, Thoraxcenter, Rotterdam, The Netherlands; 8. Department of Cardiology, Academic Medical Center, University of Amsterdam, Amsterdam, Netherlands; 9. Imperial College London, London, United Kingdom

R. Torii and E. Tenekecioglu contributed equally as first co-authors.

Two patients received 3.0×18 mm AbsorbTM bioresorbable vascular scaffolds (Abbott Vascular, Santa Clara, CA, USA), one in the left anterior descending coronary artery, the other in the circumflex coronary artery. Post-implantation OCT (pullback speed: 20 mm/s, acquisition rate: 200 frames/s) and angiographic data were fused to reconstruct the coronary anatomy, and computational fluid dynamic (CFD) techniques were used to simulate Newtonian steady blood flow and estimate endothelial shear stress (ESS) distributions¹. **Panels A, B, C & P1** show underexpansion of the scaffold (mean expansion index: 0.51). **Panels D, E, F & P2** show an overexpanded bioresorbable scaffold (mean expansion index: 1.32).

In the CFD model of the underexpanded case (**Panel C**), high ESS (in red) was noted on top of the struts which disrupted the flow, creating recirculation zones and low ESS (in dark blue) in the inter-strut zones. Scaffold underexpansion caused a “step-down” at the proximal edge of the scaffolded segment (**Panel P1**, black box in **Panel C**). On the five-year OCT, there was attenuation of the step-down appearance with normalised ESS in the


proximal edge segment (**Panels A', B', C' & P1'**); the luminal surface was smoother and overall the shear stress was more homogeneous and physiological (1.5-3.0 Pa).

In the CFD model of the overexpanded case, low ESS was detected not only in the inter-strut areas but also on top of the struts. Scaffold overexpansion caused a “step-up” at the proximal edge of the scaffolded segment. At the five-year follow-up, the step-up became less prominent and the areas of very low shear stress regressed considerably (**Panels D', E', F' & P2'**).


These two cases of overexpansion and underexpansion at baseline resulted acutely in two different shear stress distributions. Both increased and decreased ESS appear to induce a biological mechano-transduction process that aims at normalising ESS levels at long-term follow-up to values close to the physiological ranges (1.5-2.5 Pa). The mechanism of “normalisation” seems to be related to a dynamic remodelling, which presumably resulted from shear stress, wall stress, cyclic strain and other important biologic factors^{2,3}.

*Corresponding author: Imperial College London, South Kensington Campus, London, SW7 2AZ, United Kingdom.
E-mail: patrick.w.j.c.serruys@gmail.com

Underexpansion case

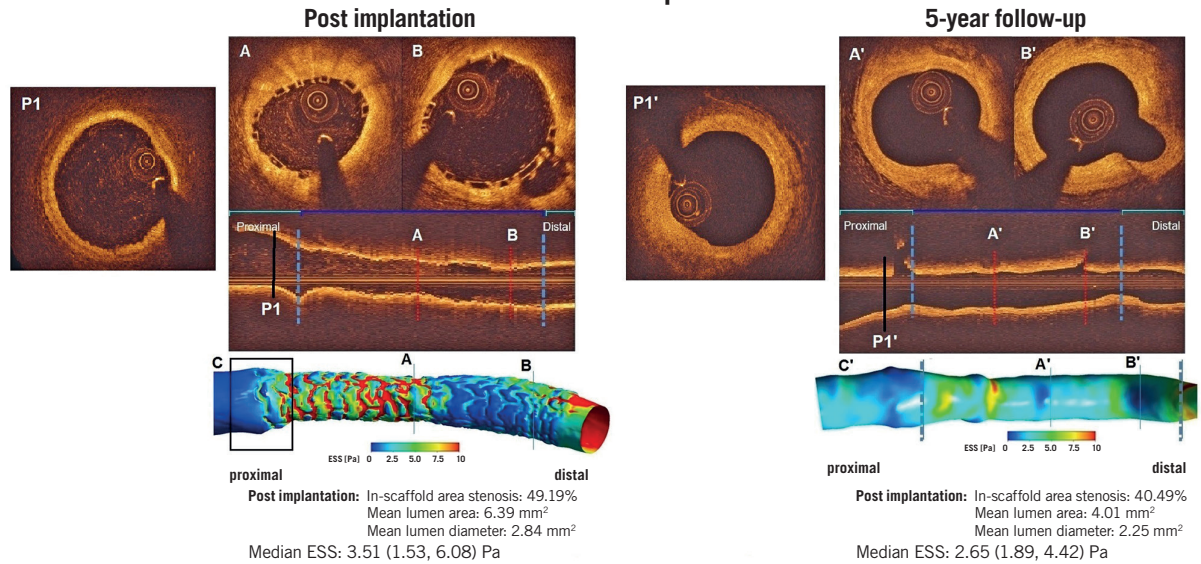

Overexpansion case

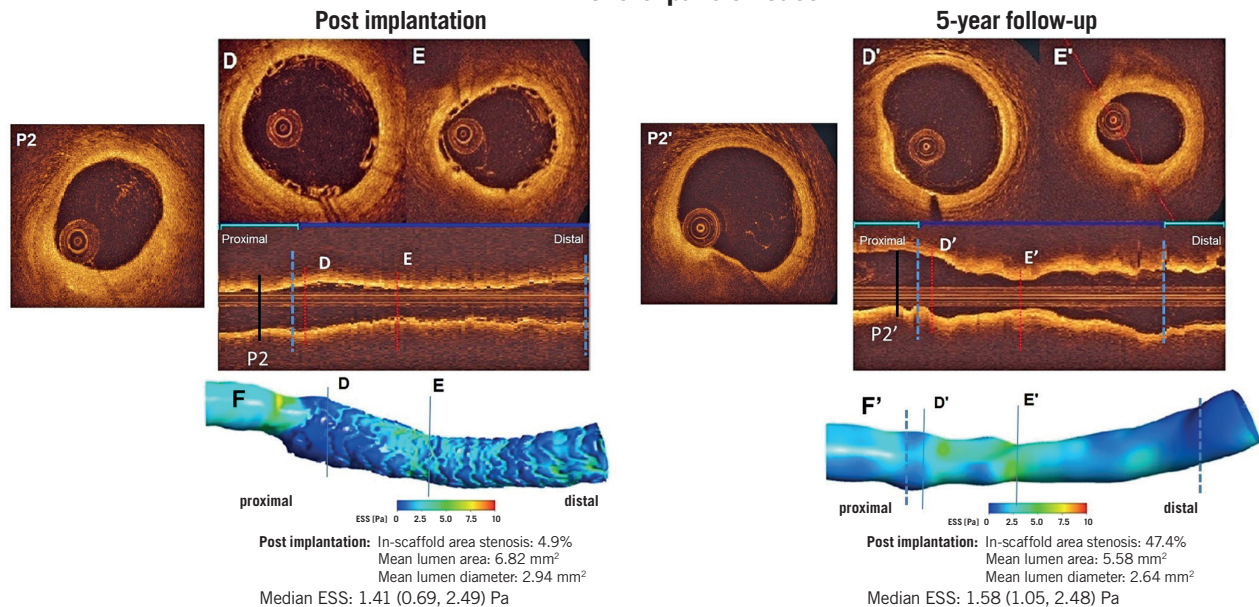

Practical implication

Underexpansion and overexpansion have been incriminated as causative factors of adverse cardiac events. However, dynamic biological interaction between vessel wall and scaffold may attenuate the adverse haemodynamic impact of overexpansion or underexpansion.

Conflict of interest statement

P.W. Serruys and Y. Onuma are members of the International Advisory Board of Abbott Vascular. The other authors have no conflicts of interest to declare.

References

1. Tenekecioglu E, Poon EK, Collet C, Thondapu V, Torii R, Bourantas CV, Zeng Y, Onuma Y, Ooi AS, Serruys PW, Barlis P. The Nidus for Possible Thrombus Formation: Insight From the

Microenvironment of Bioresorbable Vascular Scaffold. *JACC Cardiovasc Interv.* 2016;9:2167-8.

2. Koskinas KC, Chatzizisis YS, Antoniadis AP, Giannoglou GD. Role of endothelial shear stress in stent restenosis and thrombosis: pathophysiologic mechanisms and implications for clinical translation. *J Am Coll Cardiol.* 2012;59:1337-49.

3. Stone PH, Saito S, Takahashi S, Makita Y, Nakamura S, Kawasaki T, Takahashi A, Katsuki T, Nakamura S, Namiki A, Hirohata A, Matsumura T, Yamazaki S, Yokoi H, Tanaka S, Otsuji S, Yoshimachi F, Honye J, Harwood D, Reitman M, Coskun AU, Papafaklis MI, Feldman CL; PREDICTION Investigators. Prediction of progression of coronary artery disease and clinical outcomes using vascular profiling of endothelial shear stress and arterial plaque characteristics: the PREDICTION Study. *Circulation.* 2012;126:172-81.