

CLINICAL INVESTIGATIONS

Mechanism of high-speed rotational atherectomy and adjunctive balloon angioplasty revisited by quantitative coronary angiography: Edge detection versus videodensitometry

Clemens von Birgelen, MD, Victor A. Umans, MD, PhD, Carlo Di Mario, MD, PhD, David Keane MB, MRCPI, PhD, Robert Gil, MD, Francesco Prati, MD, Pim de Feyter, MD, PhD, and Patrick W. Serruys, MD, PhD *Rotterdam, The Netherlands*

High-speed rotational coronary atherectomy (RA) is primarily used to treat complex lesions. Quantitative angiographic analysis of such complex lesions by edge detection is often unsuitable, whereas videodensitometry, measuring vessel dimensions independently of the target stenosis contours, may offer potential advantages. To gain insight into the operative mechanism of RA and to study the agreement between the two quantitative angiographic methods in measuring the minimal luminal cross-sectional area, the edge detection and videodensitometry techniques were applied to coronary angiograms of 21 lesions in 19 patients with symptoms who underwent successful RA and balloon angioplasty (BA). Obstruction diameter as determined by edge detection increased from 1.00 ± 0.31 mm before intervention to 1.35 ± 0.29 mm after RA ($p < 0.001$) and further increased to 1.74 ± 0.33 mm after adjunctive BA ($p < 0.001$). The mean between-method difference (edge detection minus videodensitometry) was 0.34 mm^2 before intervention, 0.13 mm^2 after RA, and 0.09 mm^2 after adjunctive BA (not significant). The standard deviation of the differences decreased from $\pm 0.87 \text{ mm}^2$ before intervention to $\pm 0.80 \text{ mm}^2$ after RA (not significant) and increased after BA significantly to $\pm 1.21 \text{ mm}^2$ ($p < 0.05$). Thus edge detection and videodensitometry provided equivalent immediate angiographic results after RA and adjunctive BA. The good agreement after RA may reflect the operative mechanism of RA, which by ablation of noncompliant plaque material yields a circular symmetric lumen with smooth surface. The increased dis-

persion of the between-method differences observed after adjunctive BA presumably results from dissections, plaque ruptures, and loss of luminal smoothness after balloon dilatation. (AM HEART J 1995;130:405-12.)

High-speed rotational atherectomy (RA) is an interventional device that ablates and pulverizes non-compliant coronary plaque material by high-frequency rotation of a diamond-coated burr.¹ It may be used as a stand-alone procedure for treatment of coronary lesions but is frequently used as a primary device and is subsequently combined with balloon angioplasty (BA) or directional atherectomy.²⁻¹³ It has by preference been applied to diffusely diseased and calcified coronary arteries with complex lesion architecture.^{5, 9-17} To assess the results of intracoronary interventions objectively, reliably, and reproducibly, a computerized semiautomated quantification of the lumen should be applied to the cineangiograms.¹⁸⁻²⁴

There are two principal approaches of computerized angiographic analysis: edge detection and videodensitometry. Whereas edge detection is based on an automatic contour detection of the geometric vessel shape, videodensitometry is independent of luminal shape of the target stenosis and is based on the relation between the optical density of the contrast-enhanced lumen and the absolute vessel dimensions. In clinical practice edge detection is still considered the standard approach of quantitative angiographic analysis, whereas the value of videodensitometric assessments remains controversial.^{20, 22, 25-36} To gain

From Thoraxcenter, Erasmus University Rotterdam.

Dr. von Birgelen is the recipient of a fellowship of the German Research Society (DFG, Bonn, Germany).

Received for publication Dec. 28, 1994; accepted Feb. 16, 1995.

Reprint requests: Professor P.W. Serruys, MD, PhD, Cardiac Catheterization Laboratory, Thoraxcenter, Erasmus University, Bd 432, P.O. Box 1738, 3000 DR Rotterdam, The Netherlands.

Copyright © 1995 by Mosby-Year Book, Inc.

0002-8703/95/\$3.00 + 0 4/1/65048

Table 1. Edge detection before intervention, after rotational atherectomy, and after adjunctive balloon angioplasty

	Before intervention	After RA	After BA
Reference diameter (mm)	2.68 ± 0.52	2.68 ± 0.46	2.71 ± 0.49
Obstruction diameter (mm)	1.00 ± 0.31*	1.35 ± 0.29*	1.74 ± 0.33*
Diameter stenosis (%)	61.7 ± 12.2*	49.38 ± 7.41*	35.4 ± 10.12*

* $p < 0.001$ (before intervention vs after RA, before intervention vs after adjunctive BA, and after RA vs after adjunctive BA).

insight into the operative mechanism and the post-procedural luminal geometry after RA and BA and to study the agreement between the two quantitative angiographic methods in measuring the minimal luminal cross-sectional area,³⁷ edge detection and videodensitometry were applied to coronary angiograms that were acquired before intervention, after RA, and after adjunctive BA.

METHODS

Study patients and qualitative lesion characteristics.

Nineteen patients, 12 men and seven women with a mean age of 62.4 years (range, 48 to 73 years) who had 21 calcified American College of Cardiology/American Heart Association (ACC/AHA) type B2 or C lesions^{38, 39} that had been successfully treated by RA and adjunctive BA were studied. All lesions were nonostial and located in native coronary arteries, mostly with angiographic evidence of diffuse plaque calcification (18 of 21 lesions). Location of the lesion was right coronary artery (RCA) in 10 cases, left anterior descending coronary artery (LAD) in nine, and left circumflex coronary artery (LCX) in two. In two patients two distinct lesions were individually treated (lesions 9 and 10 and lesions 13 and 14, respectively). The treated segments (Table 1) are indicated according to the AHA grading system,⁴⁰ and coronary dissections are indicated according to the morphologic classification of the National Heart, Lung and Blood Institute (NHLBI).⁴¹

Description of the interventional procedure. After pretreatment was performed with 250 mg acetylsalicylic acid and 10,000 U heparin, the coronary artery ostium was intubated with 8F to 10F standard guiding catheters. Intracoronary injection of isosorbide dinitrate was performed to prevent possible coronary spasm, and a 0.009 inch Rotablator guidewire (Heart Technology Inc., Bellevue, Wash.) was advanced distal to the lesion. The rotational ablation device, an air-turbine driven burr (Rotablator, Heart Technology Inc.) of different sizes (diameter, 1.25 to 2.5 mm) with 10 μ m diamond chips on the distal portion, was tracked proximal to the lesion and then slowly advanced during high-speed rotation of the burr at 170,000 to 200,000 rpm.

Plaque material was thereby ablated and pulverized with the stepped-burr technique aiming at a maximal burr size of approximately 75% of the adjacent reference segments. After successful high-speed RA was performed, the system was exchanged for a BA catheter. To improve the

final result adjunctive balloon angioplasty⁴² was performed at the site of the artery, which had been previously treated by RA. During the entire cardiac catheterization procedure the activated clotting time (ACT) was serially measured, and intravenous heparin was administered to maintain the ACT at 300 seconds.

Angiographic image acquisition. During initial coronary angiography three views with orthogonal projections and an angle of at least 40 degrees between each were acquired. The lesion characteristics were derived from these views. Quantitative angiographic analysis was performed after RA treatment and adjunctive BA in the single worst view. To allow a reliable off-line quantification of the luminal dimensions by videodensitometry, frames with a homogeneous and complete opacification of the coronary lumen at the segment of interest were selected for analysis.

Quantitative coronary angiography. The minimal luminal area was determined by edge detection and videodensitometry. The quantitative analysis of the cineangiograms was performed off-line with the computer-assisted cardiovascular angiographic analysis system (CAAS, Pie Medical, Maastricht, The Netherlands), previously described in detail.^{30, 32, 43, 44} First, an end-diastolic cine-frame was selected for off-line analysis. A 6.9 × 6.9 mm region of interest comprising a chosen coronary segment was then selected from the 18 × 24 mm image area on the 35 mm cineframe and was digitized into a 512 × 512 pixel matrix with 258 gray levels (8 bits) with the use of a high-fidelity CCD-camera. Edge detection and videodensitometry were then performed.

Edge detection. Based on the weighted sum of the first and second derivative functions applied to the digitized brightness silhouette, automatic detection of the coronary artery contours was performed. The diameter function of the coronary artery lumen was determined by computing the shortest distances between the edge points of the left and right contours.⁴³ The interpolated reference diameter was based on a computerized estimation of the original arterial dimension at the site of the obstruction. After the procedure was performed, the diameter of the guiding catheter was measured by an electronic precision micrometer (Mitutoyo OP-1HS Tokyo, Japan; accuracy 0.001 mm). With the measured dimensions of the guiding catheter used for calibration, absolute values of the minimal diameter of the stenosis and reference vessel diameter were calculated after correction for pincushion distortion was performed. The minimal cross-sectional area of the

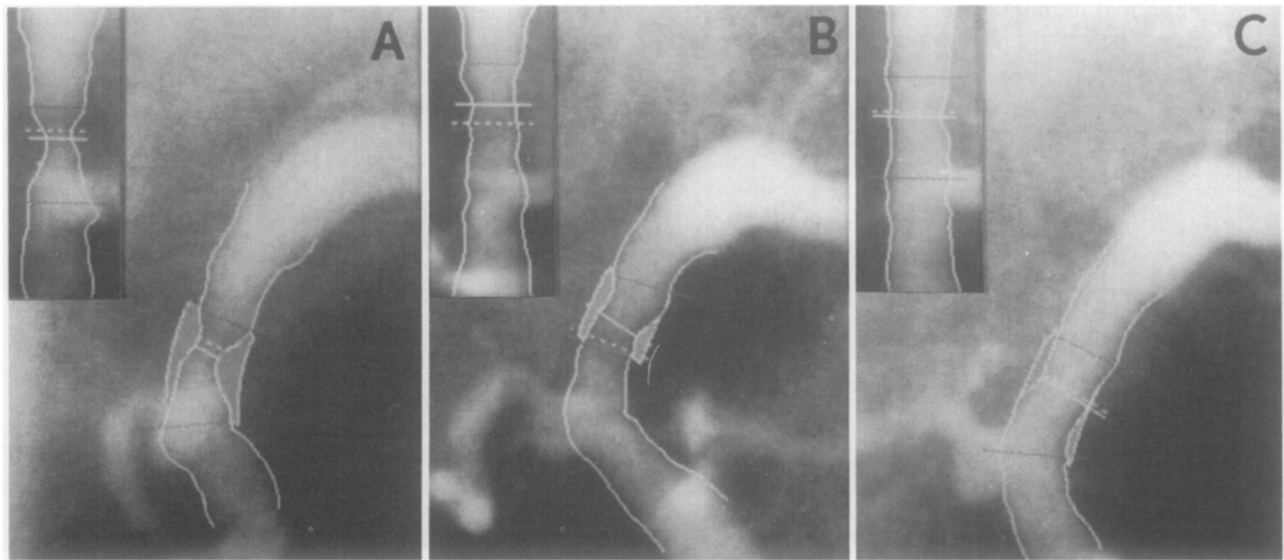


Fig. 1. Representative quantitative angiographic assessment of lesion in proximal right coronary artery before intervention (**A**), after high-speed rotational atherectomy (**B**), and after adjunctive balloon angioplasty (**C**).

narrowest segment and the interpolated percent area stenosis were subsequently calculated assuming a circular model (πr^2).

Videodensitometry. In contrast to edge detection, which considers only changes in pixel brightness, videodensitometry makes use of the absolute pixel brightness values. To obtain a cross-sectional area function of the lumen along a segment of interest from a density silhouette of an opacified coronary artery, brightness levels have to be calibrated in terms of the amount of x-ray absorption with Lambert Beer's law. Corrections for spatially variant responses in the imaging chain and processing of the cine-film were performed. The contours and diameter values of the analyzed coronary segment were obtained from the CAAS described previously. The profile of brightness of multiple scan-lines perpendicular to the local center-line direction of the coronary artery was then measured. Consequently this brightness profile was transformed by a logarithmic transfer function into an absorption profile (gross absorption). By computing the linear regression line through the background points directly right and left of the contours of the coronary silhouette, the background contribution was estimated and subtracted from the previous gross absorption profile to obtain the net cross-sectional absorption profile within the vessel contours. Thus a luminal cross-sectional area function along the analyzed coronary artery segment was obtained. Calibration of the videodensitometric area values was performed by comparing the luminal area of the reference calculated from the diameter measurements assuming a circular lumen configuration with the corresponding densitometric area values of the reference. The whole process of measuring luminal cross-sectional area by videodensitometry has previously been assessed in vitro by perspex models of coronary

artery obstructions⁴⁵ and in vivo with stenosis phantoms, which were introduced in porcine coronary arteries.²⁵

Statistics. Minimal luminal cross-sectional areas were measured by edge detection and videodensitometry in the single worst view. Mean and standard deviation of the between-method differences were determined at each of the three distinct times of angiographic assessment. Analysis of variance was performed to compare minimal luminal area measurements obtained from edge detection and videodensitometry before intervention, after rotational coronary atherectomy, and after adjunctive balloon angioplasty. When differences were found, two-tailed paired *t* tests were applied, and a statistical probability <0.05 was considered significant. Correlation coefficients (*r*) were calculated for the three distinct times of angiographic assessment to assess the strength of the relation between edge detection and videodensitometry in determining the minimal luminal cross-sectional area. According to the statistical approach of Bland and Altman,⁴⁶ the agreement between both methods was assessed by determining the mean and standard deviation of the between-method differences (edge detection minus videodensitometry). This procedure was performed at each of the three distinct times of study by computing the sum of the individual between-method differences. The variances of the between-method differences before intervention, after RA, and after BA were tested against each other with Pitman's Test.⁴⁷

RESULTS

At the three distinct times of angiographic assessment complete angiographic perfusion was found in all coronary arteries except one, which was initially occluded. The reference diameter of the analyzed

Table II. Minimal luminal cross-sectional area measurements (mm²) by edge detection and videodensitometry

Lesion no.	Vessel segment	Before intervention			After RA			After adjunctive BA		
		ED	VD	Difference	ED	VD	Difference	ED	VD	Difference
1	7	0.79	0.04	0.75	2.66	1.42	1.24	3.14	3.63	-0.49
2	1	0.49	-1.08	1.57	2.54	0.66	1.88	2.46	2.03	0.43
3	13	0.93	0.73	0.20	1.56	1.84	-0.28	2.24	3.01	-0.77
4	13	0.72	0.17	0.55	1.45	1.32	0.13	3.08	2.30	0.78
5	1	0.71	0.51	0.20	1.11	1.16	-0.05	3.33	2.77	0.56
6	6	0.87	1.04	-0.17	1.37	1.27	0.10	2.03	1.32	0.71
7	6	0.92	1.10	-0.18	0.77	1.52	-0.75	2.80	2.29	0.51
8	1	1.35	1.23	0.12	1.37	0.97	0.40	3.36	2.38	0.98
9	7	1.63	-0.71	2.34	1.19	1.21	-0.02	3.02	2.81	0.21
10	8	0.82	0.49	0.33	1.25	1.21	0.04	1.47	1.96	-0.49
11	2	0.52	0.54	-0.02	1.25	0.88	0.37	1.57	1.96	-0.39
12	1	—*	—	—	0.55	0.95	-0.40	2.11	2.00	0.11
13	2	1.47	0.44	1.03	1.58	1.06	0.52	1.47	0.45	1.02
14	3	0.53	0.43	0.10	0.87	0.46	0.41	2.60	2.88	-0.28
15	2	1.52	3.01	-1.49	3.70	5.84	-2.14	5.35	9.67	-4.32
16	2	0.75	1.35	-0.60	1.61	1.59	0.02	2.32	1.58	0.74
17	6	1.33	-0.56	1.89	1.25	1.18	0.07	1.77	0.53	1.24
18	6	0.83	1.01	-0.18	1.37	1.67	-0.30	1.86	2.78	-0.92
19	6	0.52	0.56	-0.04	1.63	1.19	0.44	1.65	1.51	0.14
20	2	0.92	1.10	-0.18	1.39	1.59	-0.20	2.75	2.17	0.58
21	7	0.49	-0.10	0.59	1.15	-0.05	1.20	1.11	-0.43	1.54
Mean		0.90	0.57	0.34	1.50	1.38	0.13	2.45	2.36	0.09
SD		0.36	0.88	0.87	0.70	1.11	0.80	0.94	1.92	1.21

ED, Edge detection; VD, videodensitometry.

*Initially occluded coronary artery.

coronary arteries was 2.68 ± 0.52 mm (range, 2.09 to 4.02 mm), and the lesion length was 7.45 ± 2.81 mm (range, 4.30 to 13.46 mm). The obstruction diameter increased from 1.00 ± 0.31 mm before intervention to 1.35 ± 0.29 mm after RA ($p < 0.001$) (Table I). After adjunctive BA was performed, the obstruction diameter was further enlarged to 1.74 ± 0.33 mm ($p < 0.001$). Interventional therapy reduced the diameter stenosis from $61.7\% \pm 12.2\%$ before therapy to $49.38\% \pm 7.41\%$ after RA ($p < 0.001$) and to $35.4\% \pm 10.12\%$ after adjunctive BA ($p < 0.001$) (Fig. 1).

In Table II the individual data of the minimal luminal cross-sectional area measured by edge detection and videodensitometry and the individual and mean between-method differences are presented for the three distinct times of angiographic measurement. The agreement between both diagnostic methods before and after RA and after BA is illustrated in Fig. 2. At each of the three times of angiographic study, minimal luminal cross-sectional area was determined to be greater by edge detection than by videodensitometry. Mean difference was lower after RA and after adjunctive BA (0.13 mm² and 0.09 mm², respectively) compared with preintervention (0.34 mm²). The standard deviation of the between-method

differences, representing the variability, decreased from 0.87 mm² before intervention to 0.80 mm² after RA (not significant). After adjunctive BA was performed, the standard deviation of the between-method differences increased significantly to 1.21 mm² (after RA vs after BA, $p < 0.05$). The correlation coefficient r of measurements by edge detection and videodensitometry increased from 0.22 before intervention to 0.70 after RA and to 0.86 after adjunctive BA. In all the cineangiograms no evidence of dissection was seen after RA was performed, but after adjunctive BA was performed, six (29%) of the previously dilated coronary segments showed characteristics of coronary dissection (three NHLBI dissection-type A, two type B, and one type D).

DISCUSSION

Two findings of this study should be emphasized. First, no significant difference of the mean between-method difference (edge detection minus videodensitometry) was seen after RA and after adjunctive BA were performed. Second, the standard deviation of the between-method differences increased significantly after BA was performed. These results may well reflect the operative mechanisms of the two devices, but the accuracy of the two quantitative

angiographic techniques cannot be determined and compared, because the true dimension of the vessels is unknown.^{48, 49}

Limitations of videodensitometry. In some cases videodensitometry provides negative values of the minimal luminal cross-sectional area. Negative values are more frequently found in coronary angiograms with side-branches or other radiopaque structures, interfering with the densitometric measurements by increasing the brightness profile of the reference segment. This overestimation of the reference brightness profile results in an underestimation of the minimal luminal cross-sectional area.²⁶ In this study negative values were more frequently found during the angiographic assessment before intervention, explaining the positive value of the mean between-method difference (edge detection minus videodensitometry). This finding concurs with previous reports that describe an increased incidence of negative values of minimal luminal cross-sectional area obtained from videodensitometry in smaller luminal dimensions.²⁶ In this study only one negative value of the minimal luminal cross-sectional area was obtained after RA and after adjunctive BA, respectively. This limitation of videodensitometry should soon be overcome by the incorporation of a background subtraction algorithm that corrects for the contribution of side-branches to the brightness intensity.⁵⁰

Quantitative coronary angiography in complex lesions. The low correlation of the quantitative angiographic measurements before intervention was striking. Several reasons such as the high rate of complex and narrow lesions in small, calcified, and tortuous coronary arteries and the higher incidence of negative values of minimal luminal cross-sectional area before intervention might be responsible for this finding.⁵¹ A new approach in quantitative coronary angiography is the gradient field transform. With the use of this new algorithm promising results in the quantification of complex coronary artery lesions have recently been reported.⁵²

Mechanism of rotational atherectomy. Edge detection is a quantitative angiographic method that is based on a computerized detection of the geometric contours of the vessel lumen, whereas videodensitometry operates independently of the geometric stenosis profile by using the optical density of the opacified coronary artery.^{27, 29, 30, 32, 35, 50} Differences between the results obtained by the two methods are less likely to be expected in a circular symmetric lumen, because luminal circularity is an elementary assumption in the calculation of minimal luminal cross-sectional area by edge detection in a single

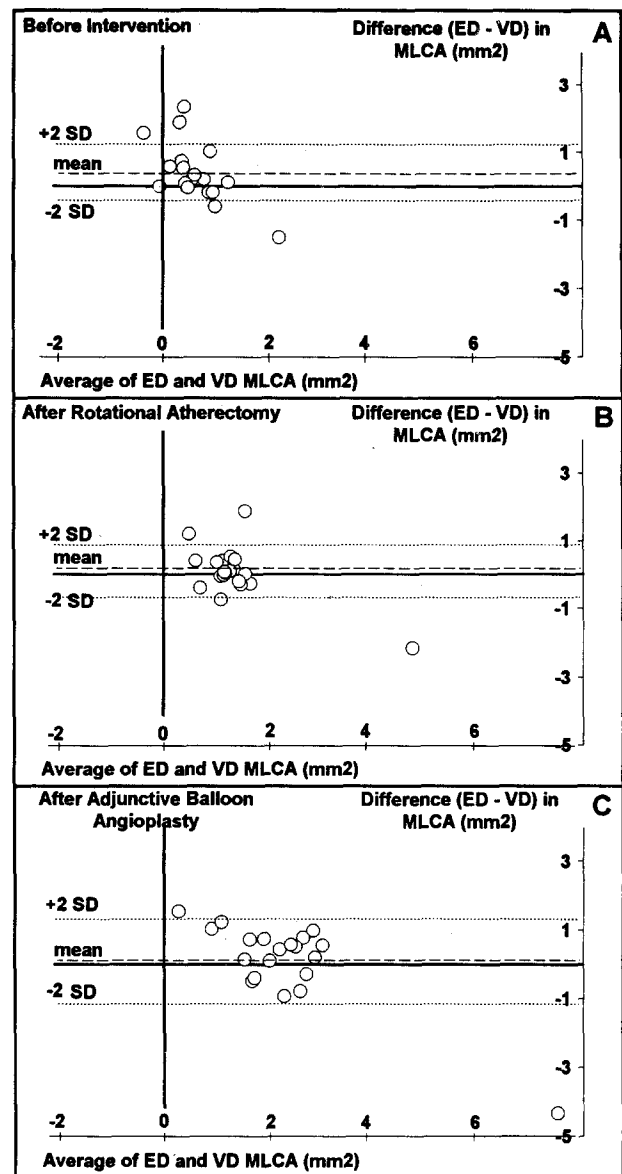


Fig. 2. Agreement of edge detection (ED) and videodensitometry (VD) in measuring minimal luminal cross-sectional area (MLCA). Mean between-method difference (ED minus VD) was lower after rotational atherectomy (B) and adjunctive balloon angioplasty (C) (0.13 mm² and 0.09 mm², respectively) compared with before intervention (A) (0.84 mm²). Standard deviation (SD) of between-method differences after rotational atherectomy remained similar to before intervention (0.80 mm² and 0.87 mm², respectively), whereas significant increase ($p < 0.05$) was found after adjunctive balloon angioplasty (1.21 mm²).

view. Thus less discrepancy between edge detection and videodensitometry was expected after plaque ablation by RA, and accordingly, good agreement of the two quantitative angiographic methods was found after RA. The presumption that the good

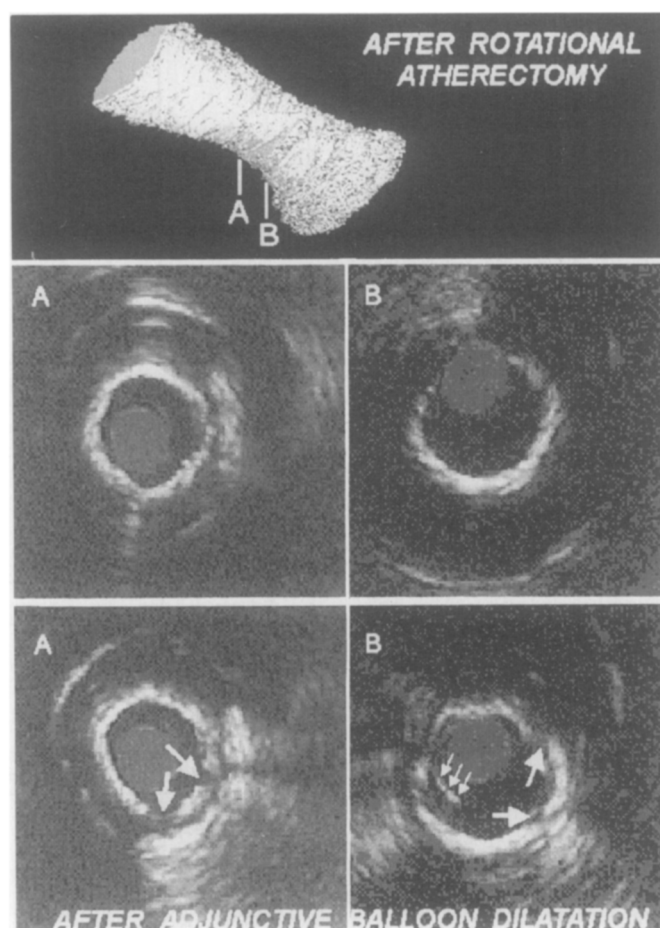


Fig. 3. Example of stenotic, circumferentially calcified proximal segment of left anterior descending coronary artery treated by rotational atherectomy and adjunctive balloon angioplasty. Intravascular ultrasound (IVUS) study reflects operative mechanism of both interventional techniques. Positions of mid-stenotic (A) and proximal (B) cross-sections, displayed in *mid* and *lower* panels, are indicated in three-dimensional IVUS lumen cast (*upper panel*), reconstructed from images acquired during motorized pull-back of IVUS catheter after rotational atherectomy. In cross-sectional images and in lumen cast, relatively smooth and circular lumen shape was found, whereas adjunctive balloon dilatation resulted in plaque rupture and dissection (*large arrowheads*) and intimal flaps (*small arrowheads*).

agreement resulted from plaque ablation providing a circular lumen shape with a smooth surface,⁵³ as confirmed by intracoronary ultrasonography^{7, 54} (Fig. 3), is supported by our previous observations describing increased agreement and correlation of the two angiographic techniques after coronary stenting.³²

Mechanism of adjunctive balloon dilatation. In this study the incidence of angiographically detected dissection after adjunctive BA was similar to that observed after primary BA.^{55, 56} Dissections are less frequent after RA than after BA,¹¹ and in the Rotational Atherectomy Multicenter Registry of 709 patients, dissections were found in 10.5% of cases.¹² Adjunctive BA increases the incidence of dissections

after RA,⁵⁷ but on the other hand BA can be used for management of coronary dissections after RA.⁹ Because the main operative mechanism of BA is rupture and dissection of the atherosclerotic plaque, a less circular and less smooth vessel shape would be expected after balloon dilatation, thus explaining the increased standard deviation of the between-method differences found after adjunctive BA. This increased variability of the between-method differences after adjunctive BA is in accordance with our previous studies performed after BA.^{30, 32}

Conclusions. When the immediate results after RA and adjunctive BA are assessed, edge detection and videodensitometry provide equivalent information. As with previous clinical studies investigating the

dimension of coronary lesions, the true absolute size of the coronary vessels is unknown, and it is thus not possible to define whether the accuracy of one of the techniques is superior to the other. Good agreement of edge detection and videodensitometry was found after RA, reflecting the operative mechanism of RA, which provides a circular lumen shape with a smooth surface by ablation and pulverization of noncompliant plaque material. Adjunctive BA further enlarged the minimal luminal cross-sectional area but also increased the variability of the differences between the measurements provided by edge detection and videodensitometry. This increase is believed to result from dissections, plaque ruptures, and loss of luminal smoothness produced by balloon angioplasty.

REFERENCES

- Hansen DD, Auth DC, Vracko R, Ritchie JL. Rotational atherectomy in atherosclerotic rabbit iliac arteries. *AM HEART J* 1988;15:160-5.
- Bertrand ME, Lablanche JM, Leroy F, Bateurs C, de Jagere P, Serruys PW, Meyer J, Dietz U, Erbel R. Percutaneous transluminal coronary rotary ablation with rotablator (European experience). *Am J Cardiol* 1992;69:470-4.
- Brogan WC, Popma JJ, Pichard AD, Satler LF, Kent KM, Mintz GS, Leon MB. Rotational coronary atherectomy after unsuccessful coronary balloon angioplasty. *Am J Cardiol* 1993;71:794-8.
- Dietz U, Erbel R, Rupprecht HJ, Weidmann S, Meyer J. High frequency rotational ablation: an alternative in treating coronary artery stenoses and occlusions. *Br Heart J* 1993;70:327-36.
- Ellis EG, Popma JJ, Buchbinder M, Franco I, Leon MB, Kent KM, Pichard AD, Satler LF, Topol EJ, Whitlow PL. Relation of clinical presentation, stenosis morphology, and operator technique to the procedural results of rotational atherectomy and rotational atherectomy-facilitated angioplasty. *Circulation* 1994;89:882-92.
- Jackman JD Jr, Hermiller JB, Sketch MH Jr, Davidson CJ, Tchong JE, Phillips HR, Stack RS. Combined rotational and directional atherectomy guided by intravascular ultrasound in an occluded vein graft. *AM HEART J* 1992;124:214-6.
- Kovach JA, Mintz GS, Pichard AD, Kent KM, Popma JJ, Satler LF, Leon MB. Sequential intravascular ultrasound characterization of the mechanisms of rotational atherectomy and adjunct balloon angioplasty. *J Am Coll Cardiol* 1993;22:1024-32.
- Mintz GS, Pichard AD, Popma JJ, Kent KM, Satler LF, Leon MB. Preliminary experience with adjunct directional coronary atherectomy after high-speed rotational atherectomy in the treatment of calcific coronary artery disease. *Am J Cardiol* 1993;71:799-804.
- Safian RD, Niazi KA, Strzelecki M, Lichtenberg A, May MA, Juran N, Freed M, Ramos R, Gangadharan V, Grines CL, O'Neill WW. Detailed angiographic analysis of high-speed mechanical rotational atherectomy in human coronary arteries. *Circulation* 1993;88:961-8.
- Stertz SH, Rosenblum J, Shaw RE, Sugeng I, Hidalgo B, Ryan C, Hansell HN, Murphy MC, Myler RK. Coronary rotational ablation: initial experience in 302 procedures. *J Am Coll Cardiol* 1993;21:287-95.
- Stertz SH, Pomerantsev EV, Shaw RE, Boucher RA, Millhouse F, Zipkin RE, Hidalgo BO, Murphy MC, Hansell HN, Myler RK. Comparative study of the angiographic morphology of coronary artery lesions treated with PTCA, directional coronary atherectomy, or high-speed rotational ablation. *Cathet Cardiovasc Diagn* 1994;33:1-9.
- Warth DC, Leon MB, O'Neill W, Zacca N, Polissar NL, Buchbinder M. Rotational atherectomy multicenter registry: acute results, complications and 6-month angiographic follow-up in 709 patients. *J Am Coll Cardiol* 1994;24:641-8.
- Zimarino M, Corcos T, Favereau X, Commeau P, Tamburino C, Spaulding C, Guerin Y. Rotational coronary atherectomy with adjunctive balloon angioplasty for treatment of ostial lesions. *Cathet Cardiovasc Diagn* 1994;33:22-7.
- Koller PT, Freed M, Grines CL, O'Neill W. Success, complications, and restenosis following rotational and transluminal extraction atherectomy of ostial stenoses. *Cathet Cardiovasc Diagn* 1994;31:255-60.
- MacIsaac AI, Whitlow PL, Cowley MJ, Buchbinder M. Coronary rotational atherectomy for calcified and non calcified lesions: final registry analysis [Abstract]. *J Am Coll Cardiol* 1994;23:285A.
- Teirstein PS, Warth DC, Najmul HAQ, Jenkins NS, McCowan LC, Aubanel-Reidel P, Morris N, Ginsburg R. High speed rotational coronary atherectomy for patients with diffuse coronary artery disease. *J Am Coll Cardiol* 1991;18:1694-701.
- Tuzcu EM, Whitlow PL, De Franco AC, Raymond RE, Elliot J, Lefkowitz J, Guyer S, Franco I, Ellis SG, Nissen SE. Comparison of DCA and Rotablation by intravascular ultrasound: mechanism and extent of plaque removal [Abstract]. *J Am Coll Cardiol* 1994;23:301A.
- Applegate RJ, Herrington DM, Little WC. Coronary angiography: more than meets the eye. *Circulation* 1993;87:1399-401.
- Fleming RM, Kirkeeide RL, Smalling RW, Gould KL. Patterns in visual interpretation of coronary arteriograms as detected by quantitative coronary arteriography. *J Am Coll Cardiol* 1991;18:945-51.
- Gould KL. Quantitative coronary angiography. In: Gould KL, ed. *Coronary artery stenosis*. 1st ed. New York: Elsevier Science Publishing, 1991:93-107.
- Herrington DM, Siebes M, Sokol DK, Siu CO, Walford GD. Variability in measures of coronary lumen dimensions using quantitative coronary angiography. *J Am Coll Cardiol* 1993;22:1068-74.
- Mancini GBJ. Quantitative coronary arteriographic methods in the interventional catheterization laboratory: an update and perspective. *J Am Coll Cardiol* 1991;17:23B-33B.
- Mancini GBJ, Bourassa MG, Williamson PR, Leclerc G, DeBoe SF, Pitt B, Lesperance J. Prognostic importance of quantitative analysis of coronary cineangiograms. *Am J Cardiol* 1992;69:1022-7.
- Waters D, Craven TE, Lesperance J. Prognostic significance of progression of coronary atherosclerosis. *Circulation* 1993;87:1067-75.
- Di Mario C, Haase J, den Boer A, Reiber JHC, Serruys PW. Edge detection versus densitometry in the quantitative assessment of stenosis phantoms: an in vivo comparison in porcine coronary arteries. *AM HEART J* 1992;124:1181-9.
- Escaned J, Haase J, Foley DP, Di Mario C, Den Boer A, Montauban van Swijndregt E, Serruys PW. Videodensitometry in percutaneous coronary interventions: a critical appraisal of its contributions and limitations. In: Serruys PW, Foley DP, de Feyter PJ eds. *Quantitative coronary angiography in clinical practice*. Dordrecht-Boston-London: Kluwer Academic Publishers, 1994:69-87.
- Herrold EM, Goldberg HL, Borer JS, Wong K, Moses JW. Relative insensitivity of densitometric stenosis measurement to lumen edge determination. *J Am Coll Cardiol* 1990;15:1570-77.
- Nichols AB, Berke AD, Han J, Reison DS, Watson RM, Powers ER. Cinevideodensitometric analysis of the effect of coronary angioplasty on coronary stenotic dimensions. *AM HEART J* 1988;115:722-32.
- Sanz ML, Mancini GBJ, LeFree MT, Mickelson JK, Starling MR, Vogel RA, Topol EJ. Variability of quantitative digital subtraction coronary angioplasty. *Am J Cardiol* 1987;60:55-60.
- Serruys PW, Reiber JHC, Wijns W, v.d. Brand M, Kooijman CJ, ten Katen HJ, Hugenholtz PG. Assessment of percutaneous transluminal coronary angioplasty by quantitative coronary angioplasty by quantitative coronary angiography: diameter versus densitometric area measurements. *Am J Cardiol* 1984;54:482-8.
- Silver KH, Buczeck JA, Esser PD, Nichols AB. Quantitative analysis of coronary angiograms by microprocessor cinevideodensitometry. *Cathet Cardiovasc Diagn* 1987;13:291-300.
- Strauss BH, Juilliere Y, Rensing BJ, Reiber JHC, Serruys PW. Edge detection versus densitometry for assessing coronary stenting quantitatively. *Am J Cardiol* 1991;67:484-90.
- Theron HT, Lambert CR, Pepine CJ. Videodensitometric versus digital calipers for quantitative coronary angiography. *Am J Cardiol* 1990;66:1186-90.
- Tobis J, Nalcioğlu O, Johnston WD, Qu L, Reese T, Henry WL. Videodensitometric determination of minimum coronary diameter before and after angioplasty. *Am J Cardiol* 1987;59:38-44.
- Umans VA, Strauss BH, de Feyter PJ, Serruys PW. Edge detection versus videodensitometry for quantitative angiographic assessment of directional coronary atherectomy. *Am J Cardiol* 1991;68:534-39.

36. Whiting JS, Pfaff JM, Eigler NL. Advantages and limitations of videodensitometry in quantitative coronary angiography. In: Reiber JHC, Serruys PW, eds. Quantitative coronary angiography. Dordrecht-Boston-London: Kluwer Academic Publishers, 1991:43-54.
37. Harrison DG, White CW, Hiratzka LF, Doty DB, Barnes DH, Eastham CL, Marcus ML. The value of lesion cross-sectional area determined by quantitative coronary angiography in assessing the physiologic significance of proximal left anterior descending arterial stenoses. *Circulation* 1984;69:1111-9.
38. Ellis SG, Vandormael MG, Cowley MJ, Di Sciascio G, Deligonul U, Topol EJ, Bulle TM, and the multivessel angioplasty prognosis study group. Coronary morphologic and clinical determinants of procedural outcome with angioplasty for multivessel coronary disease. *Circulation* 1990;82:1193-202.
39. Ryan TJ, Faxon DP, Kennedy JW, King SB III, Loop FD, Peterson KL, Reeves TJ, Williams DO, Winters WL Jr. Guidelines for percutaneous transluminal coronary angioplasty: a report of the American College of Cardiology/American Heart Association Task Force on assessment of diagnostic and therapeutic cardiovascular procedures (subcommittee on percutaneous transluminal coronary angioplasty). *J Am Coll Cardiol* 1988;12:529-45 and *Circulation* 1988;78:486-502.
40. Austen WG, Edwards JE, Frye RL, Gensini GG, Gott VL, Griffith LSC, McGoon DC, Murphy ML, Roe BB. A reporting system in patients evaluated for grading of coronary artery disease. Report of the Ad Hoc Committee for Grading Coronary Artery Disease, Council on Cardiovascular Surgery, American Heart Association. *Circulation* 1975;5:609-16.
41. Huber MS, Fishman Mooney JF, Madison J, Mooney MR. Use of a morphologic classification to predict clinical outcome after dissection from coronary angioplasty. *Am J Cardiol* 1991;68:467-71.
42. Buchbinder M, O'Neill, Warth D, Zacca N, Dietz U, Bertrand ME, Fourrier JL, Leon MB. Percutaneous coronary rotational ablation using the rotablator: results of a multicenter study. *Circulation*; 1990; 82:III-309.
43. Reiber JHC, Kooijman CJ, Slager CJ, Gerbrands JJ, Schuurbijs JHC, den Boer A, Wijns W, Serruys PW, Hugenholtz PG. Coronary artery dimensions from cineangiogram: methodology and validation of a computer-assisted analysis procedure. *Comp Cardiol* 1984;131-41.
44. Di Mario C, Haase J, Escaned J, Montauban van Swijndregt E, Serruys PW. Validation of videodensitometry in the assessment of stenosis phantoms: an in vitro and in vivo study. In: Serruys PW, Foley DP, de Feyter PJ, eds. Quantitative coronary angiography in clinical practice. Dordrecht-Boston-London: Kluwer Academic Publishers, 1994:51-68.
45. Haase J, Keane D, Di Mario C, Escaned J, Slager CJ, Serruys PW. How reliable are geometric coronary measurements? In vitro and in vivo validation of digital and cinefilm-based quantitative coronary analysis systems. In: Serruys PW, Foley DP, de Feyter PJ, eds. Quantitative coronary angiography in clinical practice. Dordrecht-Boston-London: Kluwer Academic Publishers, 1994:27-49.
46. Bland JM, Altman DG. Statistical methods for assessing agreement between two methods of clinical measurement. *Lancet* 1986;1:307-10.
47. Pitman EJG. A note on normal correlation. *Biometrika* 1939;31:9-12.
48. Keane D, Haase J, Slager CJ, Montauban van Swijndregt E, Lehmann KG, Ozaki Y, Di Mario C, Kirkeeide R, Serruys PW. Comparative validation of quantitative coronary angiography systems: results and implications from a multicenter study using a standardized approach. *Circulation*; 1995;91:2174-83.
49. Keane D, Serruys PW. Quantitative coronary angiography: an integral component of interventional cardiology. In: Topol EJ, Serruys PW, eds. Current review of interventional cardiology. 2nd ed. Current Medicine, Philadelphia: 1995:205-33.
50. Gronenschild E, Janssen J, Tijdens F. CAAS II: a second generation system for off-line and on-line quantitative coronary angiography. *Cathet Cardiovasc Diagn* 1994;33:61-75.
51. Gurley JC, Nissen SE, Booyh DC, De Maria AN. Influence of operator and patient-dependent variables on the suitability of automated quantitative coronary arteriography for routine clinical use. *J Am Coll Cardiol* 1992;19:1137-43.
52. Zwet van der PMJ, Reiber JHC. A new approach for the quantification of complex lesion morphology: the gradient field transform; basic principles and validation results. *J Am Coll Cardiol* 1994;24:216-24.
53. McFadden EP, Lablanche JM, Bateurs C, Quandalle P, Bertrand ME. Rotational atherectomy—an overview. In: Reiber JHC, Serruys PW, eds. Progress in quantitative coronary arteriography. Dordrecht-Boston-London: Kluwer Academic Publishers, 1994:353-366.
54. Mintz G, Potkin B, Keren G, Satler LF, Pichard AD, Kent KM, Popma JJ, Leon MB. Intravascular ultrasound evaluation of the effect of rotational atherectomy in obstructive atherosclerotic coronary disease. *Circulation* 1992;86:1383-93.
55. Hermans WRM, Rensing BJ, Foley DP, Deckers JW, Rutsch W, Emanuelsson H, Danchin N, Wijns W, Chappuis F, Serruys PW. Therapeutic dissection after successful coronary angioplasty: no influence on restenosis or on clinical outcome: a study in 693 patients. *J Am Coll Cardiol* 1992;20:767-80.
56. Leimgruber PP, Roubin GS, Anderson HV, et al. Influence of intimal dissection on restenosis after successful coronary angioplasty. *Circulation* 1985;72:530-5.
57. Pomerantsev EV, Stertz SH, Yeung AC, Oesterle SN, Botas J, Shaw RE. High speed rotational atherectomy: assessment of spasm and elastic recoil. *Circulation* 1994;90:I-213.